



DETERMINATION OF ACCURACY OF ELECTRONIC APEX LOCATOR IN THE FUNCTION OF DIFFERENT EMPLOYMENT PROTOCOLS IN VITAL AND NON VITAL TEETH : AN IN-VIVO STUDY

Dental Science

Dr. Joe Antony George*	Rajarajeswari Dental College & Hospital, Bangalore Affiliated To Rajiv Gandhi University Of Health Sciences *Corresponding Author
Dr. K. J Nandakishore	Rajarajeswari Dental College & Hospital, Bangalore Affiliated To Rajiv Gandhi University Of Health Sciences
Dr. Geeta I. B	Rajarajeswari Dental College & Hospital, Bangalore Affiliated To Rajiv Gandhi University Of Health Sciences
Dr. Mohammed Idris	Rajarajeswari Dental College & Hospital, Bangalore Affiliated To Rajiv Gandhi University Of Health Sciences
Dr. Sachin Sunny Otta	Rajarajeswari Dental College & Hospital, Bangalore Affiliated To Rajiv Gandhi University Of Health Sciences

ABSTRACT

Introduction: Accurate working length determination is a crucial factor that influences the outcome of root canal therapy. Root canal length determination is commonly performed using radiographic methods or apex locator.

Aim: Determination of accuracy of electronic apex locator in the function of different employment protocols in vital and non vital teeth.

Methodology: 20 patients are selected for root canal treatment. The patients are divided into 2 groups based on vital and non vital teeth. Working length determination is done by using an apex locator. The accuracy of working length determined is confirmed using digital radiography. The tooth to be treated is anaesthetised and isolated with rubber dam. Access opening is done and a 10k file is used for determining the working length using an electronic apex locator. As the file progress in, the reading is noted. Two employment protocols are used:

1. File stops at the apex and coming back to 0.5.
2. File goes beyond zero and coming back to 0.5.

Result: There is no statistical significant difference between the two protocols regardless of the conditions used. Protocol 2 showed favourable results when compared with protocol 1

KEYWORDS

apex loator, apical foramen

INTRODUCTION

Accurate working length determination is a prerequisite for the success of root canal treatment. In endodontics, the working length is defined as the distance from coronal reference point to the point at which chemo mechanical preparation and obturation has to terminate¹. Apical anatomy determines the termination of the root canal instrumentation and filling. The cemento dentinal junction which is also described as apical constriction is the anatomical and histological landmark where the periodontal ligament begins and pulp ends².

One of the major problems in endodontic treatment has always been identification and maintenance of the biological length of the root canal system³. Different methods have been used for locating the position of canal terminus and measuring the working length of the root canal. This includes tactile, radiographs, electronic apex locator and other adjuvant methods⁴.

The evolution of electronic apex locator has reached accuracy level of above 95 % and which is more accurate method to determine apical constriction⁵. Several studies have been dedicated to evaluate the accuracy of electronic apex locator such as pre-flaring of canals, or using different protocols that determine the insertion of the instruments until they reach some anatomic position (example: the apical foramen [AF], apical constriction, or even positions below the AF) has influence on accuracy of electronic apex locator^{6,7,8,9}. Very few studies have taken vitality into consideration in determining the working length using electronic apex locator. The readings may vary if there is any structural alterations in root apex of the nonvital teeth, electric conductivity of dentinal wall, pathological alteration in the apex of the tooth with apical periodontitis¹⁰. Also, different impedance values between necrotic pulp and vital pulp due to the destruction of periodontal ligament^{11,12} may result in erroneous readings with the electronic apex locator. Some studies have found statistically no difference in the accuracy of electronic apex locator to locate the apical constriction and apical foramen in vital and nonvital cases while some studies have found a significant difference^{11,13,14,15,16}. But as far as my knowledge, there are no study conducted for determining the accuracy

of electronic apex locator using different functional protocol (Protocol 1- file going till apex and coming back to .5. Protocol 2 - file going beyond apex and coming back to .5) used in different conditions of pulp (vital and non vital pulp).

MATERIALS AND METHODS

A total of 20 patients were selected for this in vivo study. The study subjects were recruited from a pool of patients referred to department of conservative dentistry and endodontics.

INCLUSION CRITERIA:

Single rooted tooth with mature apex, Vital and Nonvital pulp, Healthy patients without systemic disease or allergic reactions, Age group –20-35.

EXCLUSION CRITERIA:

Patient with systemic disease, Severely damaged tooth, Periodontal disease, Tooth previously undergone root canal treatment, Fractured tooth, Teeth with more than one canal, Teeth with open apex, Apical resorption, Apical pathosis, Broken crowns/carries below the level of gingiva, Patient with cardiac pacemaker, Patient with implanted electrical devices, Retreatment cases, Calcified canals, Impossibility of achieving apical patency in any canal.

METHODOLOGY

All the patients were informed of the aim and design of the study and written authorizations were obtained before their inclusion. The medical and dental history of each patient was obtained, and pulpal/periapical status were examined via periapical radiographs, periodontal evaluation, palpation, percussion, electric pulp tester, and thermal tests. The following data were collected in clinical records. The pulpal status was rechecked by testing the presence of bleeding during the endodontic access (presence of blood in the canal indicates a vital pulp).

After topical anaesthetic application the teeth were anaesthetised with local anaesthetic solution containing 2% lidocaine with 1:80000 epinephrine. Caries removal and initial access was accomplished with

sterile high speed and low speed burs. The cavity access preparation was completed, pulp tissue was removed and the canal orifice was localized. The incisal or occlusal edges were ground lightly to create stable reference points for the rubber stops on the root canal files. The canal patency was determined with a sterile stainless steel k file size 10. The coronal part of each canal was flared with gates glidden drills and then each canal was irrigated with 2.5% NaOCl solution Afterwards , patients were randomly assigned to 4 groups during working length determination in vital and non vital teeth using electronic apex locator.

Group 1=File goes beyond zero +0.5(red zone with continuous beep) and coming back to -0.5(green zone) as indicated in the apex locator in vital tooth.

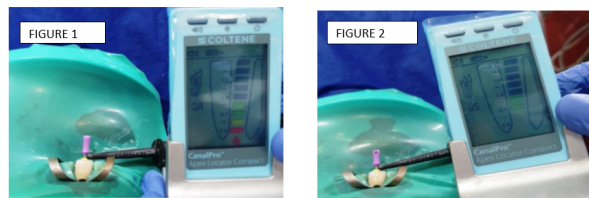


FIGURE 1 & 2: File goes beyond zero +0.5 (red zone with continuous beep) and coming back to -0.5(green zone)

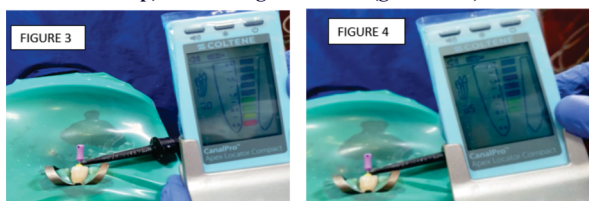


FIGURE 3 & 4: File stops at the apex (zero/red zone) and coming back to -0.5(green zone)

Group 2= File goes beyond zero +0.5 (red zone with continuous beep) and coming back to -0.5(green zone) as indicated in the apex locator in nonvital tooth.

Group 3=File stops at the apex (zero/red zone) and coming back to -0.5(green zone) as indicated in the apex locator in vital tooth.

Group 4= File stops at the apex (zero/red zone) and coming back to -0.5(green zone) as indicated in the apex locator in nonvital tooth.

The file is stabilized in patients mouth and a digital radiograph is taken using clark's rule to confirm the working length of apex locator used in different protocols.




Figure 5: Working Length Confirmation Using Radiograph

STATISTICAL ANALYSIS

Descriptive analysis includes expression of errors in working length between EAL & Radiograph in terms of Mean and SD for each study group. Mann Whitney Test was used to compare the mean error between 2 protocols and between 2 different teeth condition. The level of significance [P-Value] was set at $P < 0.05$.

RESULTS

Comparison of mean Error between 2 protocols in Vital Teeth using Mann Whitney Test					
Protocols	N	Mean	SD	Mean Diff	P-Value
Protocol 1	5	0.30	0.45		
Protocol 2	5	0.00	0.00	0.30	0.14

Note: Protocol 1 - Going till apex & coming back to 0.5
Protocol 2 - Going beyond apex & coming back to 0.5

Comparison of mean Error between Vital and Non-Vital Teeth under Protocol 1 using Mann Whitney Test					
Teeth	N	Mean	SD	Mean Diff	P-Value
Vital	5	0.30	0.45		
Non-Vital	5	0.50	0.87	-0.20	0.91

Comparison of mean Error between Vital and Non-Vital Teeth under Protocol 2 using Mann Whitney Test					
Teeth	N	Mean	SD	Mean Diff	P-Value
Vital	5	0.00	0.00		
Non-Vital	5	0.00	0.00	0.00	--

TABLE 1: COMPARISON OF MEAN ERROR BETWEEN 2

PROTOCOLS IN VITAL AND NON VITAL TEETH USING MANN WHITNEY TEST

Comparison of mean Error between 4 groups using Kruskal Wallis Test						
Groups	N	Mean	SD	Min	Max	H
Group 1	5	0.00	0.00	0.0	0.0	4.690
Group 2	5	0.00	0.00	0.0	1.0	
Group 3	5	0.30	0.45	0.0	0.0	
Group 4	5	0.50	0.87	0.0	2.0	


Note: Group 1 - Going beyond apex and coming back to .5 in vital teeth

Group 2- going beyond apex and coming back to .5 in nonvital teeth


Group 3-going till apex and coming back to .5 in vital teeth

Group 4-going till apex and coming back to .5 in nonvital teeth

TABLE 2: COMPARISON OF MEAN ERROR BETWEEN 4 GROUPS USING KRUSKAL WALLISTEST

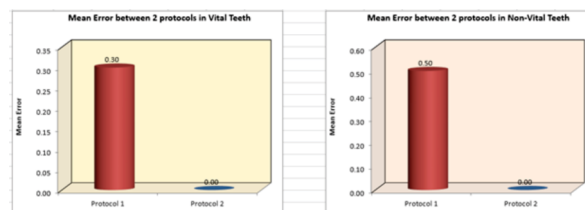

GRAPH 1: MEAN ERROR BETWEEN 2 PROTOCOLS IN VITAL AND NONVITAL TEETH

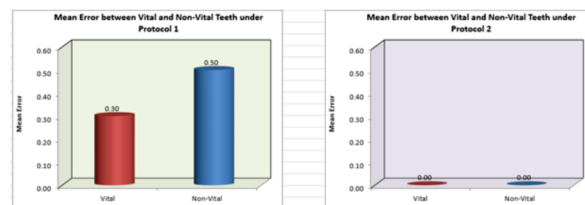

GRAPH 2: MEAN ERROR BETWEEN VITAL AND NON-VITAL TEETH UNDER 2 PROTOCOLS

Considering the tested variations, the statistical analysis pointed out that, there is no statistical significant difference between the 2 protocols (file going till apex and coming back to .5 /file going beyond apex and coming back to .5) regardless of the conditions used (vital and nonvital teeth)

However, Protocol 2 (file going beyond apex and coming back to .5) showed favourable results in both vital and non vital teeth when compared with protocol 1 (file going till apex and coming back to .5)

DISCUSSION

All measurements were conducted by the same experienced and trained operator, thus eliminating the possibility of operator bias. The evolution of electronic apex locators (EALs) has reached accuracy levels above 95% depending on the conditions in which they are used compared to other traditional methods^{17,18,19,20,21,22}. Several studies have been dedicated to evaluate the accuracy of electronic apex locators, and in these, different employment protocols have been used offering conflicting results regarding the accuracy of electronic devices¹⁵. This particular study focus on function of accuracy of electronic apex locator using different protocols in different pulp and periapical conditions. The recent apex locators works on the phenomenon of Frequency dependent comparative impedance type (third generation) ratio type (fourth generation) and dual frequency ratio type (fifth generation). Thus it works accurate irrespective of pulp and periapical conditions²³. In a study conducted by Taneja et al using different apex locators , CanalPro apex locator showed highest accuracy in all conditions in presence of irrigants, pulp/blood and open apices with accepted accuracy percentage above 90% when compared with Root ZX mini and Apex ID²⁴.

In our study, electronic apex locator reading was reconfirmed using radiographic reading. Gordon²⁵ stated that the use of apex locator alone without the use of a post operative radiograph is not a recommended practice due to large variation in tooth morphology. El Ayouti²⁶ found accuracy of about 97% in electronic apex locator, but suggested reconfirmation using radiographs.

Only single rooted straight canal tooth was included in the study.

Hoer²⁷ noted that canal curvature was found to effect on function of apex locators. Apex locators are capable of assessing apical constriction in straight and wider canals with greater accuracy as compared to narrow and curved canals²⁸.

In this study the different protocols used (file going till apex and coming back to .5 /file going beyond apex and coming back to .5) showed no statistical significant difference in accuracy of determining the working length in different pulpal conditions. Aggarwal et al in his study stated that EAL measures the location of apical constriction and apical foramen with similar accuracy in vital and nonvital teeth¹⁴. However, in our study protocol 2 (file going beyond apex and coming back to .5) showed favourable results when compared with protocol 1(file going till apex and coming back to .5). The patency is achieved with a No. 6,8,10, or 15 hand file. The average minor constriction of the apical foramen is approximately .28 mm. This is especially true if file is precurved Small hand files (No.6-15) will not cause harm. Such small hand files pass unhindered through minor constriction and are inconsequential²⁹.

CONCLUSION

There is no statistical significant difference between the two protocols regardless of vital and non-vital pulp.

Protocol 2 (going beyond and coming back to .5) showed more accurate readings compared to protocol 1 (going till apex and coming back to .5)

REFERENCES

- Glossary of Endodontic Terms. 8th edition: American Association of Endodontists:2012.
- Tuncer AK, Gerek M. Effect of working length measurement by electronic apex locator or digital radiography on postoperative pain: a randomized clinical trial. *Journal of endodontics*. 2014 Jan 1;40(1):38-41.
- Ravanshad S., Adl A., Anvar J. – Effect of working length measurement by electronic apex locator or radiography on the adequacy of final working length: a randomized clinical trial – *Journal of Endodontics*, 2010 Nov; 36(11):1753-6.
- Mohan GM, Anand GS. Accuracy of different methods of working length determination in endodontics. *IOSR journal of dental and medical science* 2013 november-december;12(4):2538
- Nekoofar MH, Ghandi MM, Hayes SJ, Dummer PM. The fundamental operating principles of electronic root canal length measurement devices. *Int Endod J* 2006;39: 595–609.
- Stool R, Urban-Klein B, Roggendorf MJ, et al. Effectiveness of four electronic apex locators to determine distance from apical foramen. *Int Endod J* 2010;43:808–17.
- Vasconcelos BC, Verissimo-Chavez RD, Vivacqua-Gomes N, et al. Ex vivo evaluation of the accuracy of electronic foramen locators in root canals with an obstructed apical foramen. *J Endod* 2015;41:1551–4.
- Vasconcelos BC, Frota LM, Souza T, et al. Evaluation of the maintenance of the apical limit during instrumentation with hybrid equipment in rotary and reciprocating modes. *J Endod* 2015;41:682–5.
- Camargo EJ, Zapata RO, Medeiros PL, et al. Influence of preflaring on the accuracy of length determination with four electronic apex locators. *J Endod* 2009;35: 1300–2.
- Piasecki L, Carneiro E, Fariniuk LF, Westphalen VP, Fiorentin MA, da Silva Neto UX, et al. Accuracy of root ZX II in locating foramen in teeth with apical periodontitis: An in vivo study. *J Endod* 2011;37:1213–6.
- Dunlap CA, Remeikis NA, BeGole EA, Rauschenberger CR. An in vivo evaluation of an electronic apex locator that uses the ratio method in vital and necrotic canals. *J Endod* 1998;24:48–50.
- Pommer O, Stamm O, Attin T. Influence of the canal contents on the electrical assisted determination of the length of root canals. *J Endod* 2002;28:83–5.
- Mayeda DL, Simon JH, Aimer DF, Finley K. In vivo measurement accuracy in vital and necrotic canals with the endex apex locator. *J Endod* 1993;19:545–8.
- Aggarwal G, Bogra P, Gupta S, Jindal A, Jain N. Determination of apical constriction and apical foramen using electronic apex locator in vivo: Comparison between vital and nonvital teeth. *Saudi Endodontic Journal*. 2018 May 1;8(2):
- Oliveira Tn, Gomes Nv, Bernardes Ra, Vivan Rr, Duarte Mah, Vasconcelos Bc. Determination of the accuracy of 5 electronic apex locators in the function of different employment protocols. *Journal of endodontics* 2017;3(39)
- Rakesh Mittal, Meenu Garg Singla, Ashima Sood, Anchal Singla. Comparative evaluation of working length determination by using conventional radiography, digital radiography and electronic apex locator. *Journal of restorative dentistry* 2015;3:75-77
- Nekoofar MH, Ghandi MM, Hayes SJ, Dummer PM. The fundamental operating principles of electronic root canal length measurement devices. *Int Endod J* 2006;39: 595–609.
- Akise E, Gratieri SD, Barletta FB, et al. Not all electronic foramen locators are accurate on teeth with enlargement apical foramina: an in vitro comparison of 5 brands. *J Endod* 2014;40:109–12.
- Martins JN, Marques D, Mata A, Carames J. Clinical efficacy of electronic apex locators: systematic review. *J Endod* 2014;40:759–77.
- Khandewal D, Ballal NV, Saraswati MV. Comparative accuracy of 2 electronic apex locators with conventional radiograph: an ex vivo study. *J Endod* 2015;41:201–4.
- Parente LA, Levin MD, Vivan RR, et al. Efficacy of electronic foramen locators in controlling root canal working length during rotary instrumentation. *Braz Dent J* 2015; 26:547–51.
- Piasecki L, Carneiro E, da Silva Neto UX, et al. The use of micro-computed tomography to determine the accuracy of 2 electronic apex locators and anatomic variations affecting their precision. *J Endod* 2016;42:1263–7.
- Amruta Khadse, Pratima Shenoi , Vandana Kokane , Rajiv Khode , Snehal Sonarkar. RElectronic Apex Locators- An overview *Indian Journal of Conservative and Endodontics*, April-June,2017;2(2):35-40
- Sonali Taneja, Mohit Kumar, Sonal Soi Sharma, Hulas G. Comparative Evaluation of Accuracy of Three Electronic Apex Locators in Different Simulated Clinical Conditions- An invitro Study. *Annals of Medical and Health Sciences Research*,2017;7:3
- Gordon MP, Chandler NP. Electronic apex locators. *International endodontic journal*. 2004 Jul;37(7):425-37.
- ElAyouti A, Weiger R, Löst C. The ability of root ZX apex locator to reduce the frequency of overestimated radiographic working length. *Journal of endodontics*. 2002 Feb 1;28(2):116-9.
- Hoer D, Attin T. The accuracy of electronic working length determination. *International endodontic journal*. 2004 Feb;37(2):125-31.]
- Sadaf D, Ahmad MZ. Accurate Measurement of Canal Length during Root Canal Treatment: An In Vivo Study. *International journal of biomedical science: IJBS*. 2015 Mar;11(1):42.
- Richard Mounce, DDS. What happens if a file goes out of the apex? Drama, trauma or non-event? *Dental Economics*, October, 2007